

Fig. 1A


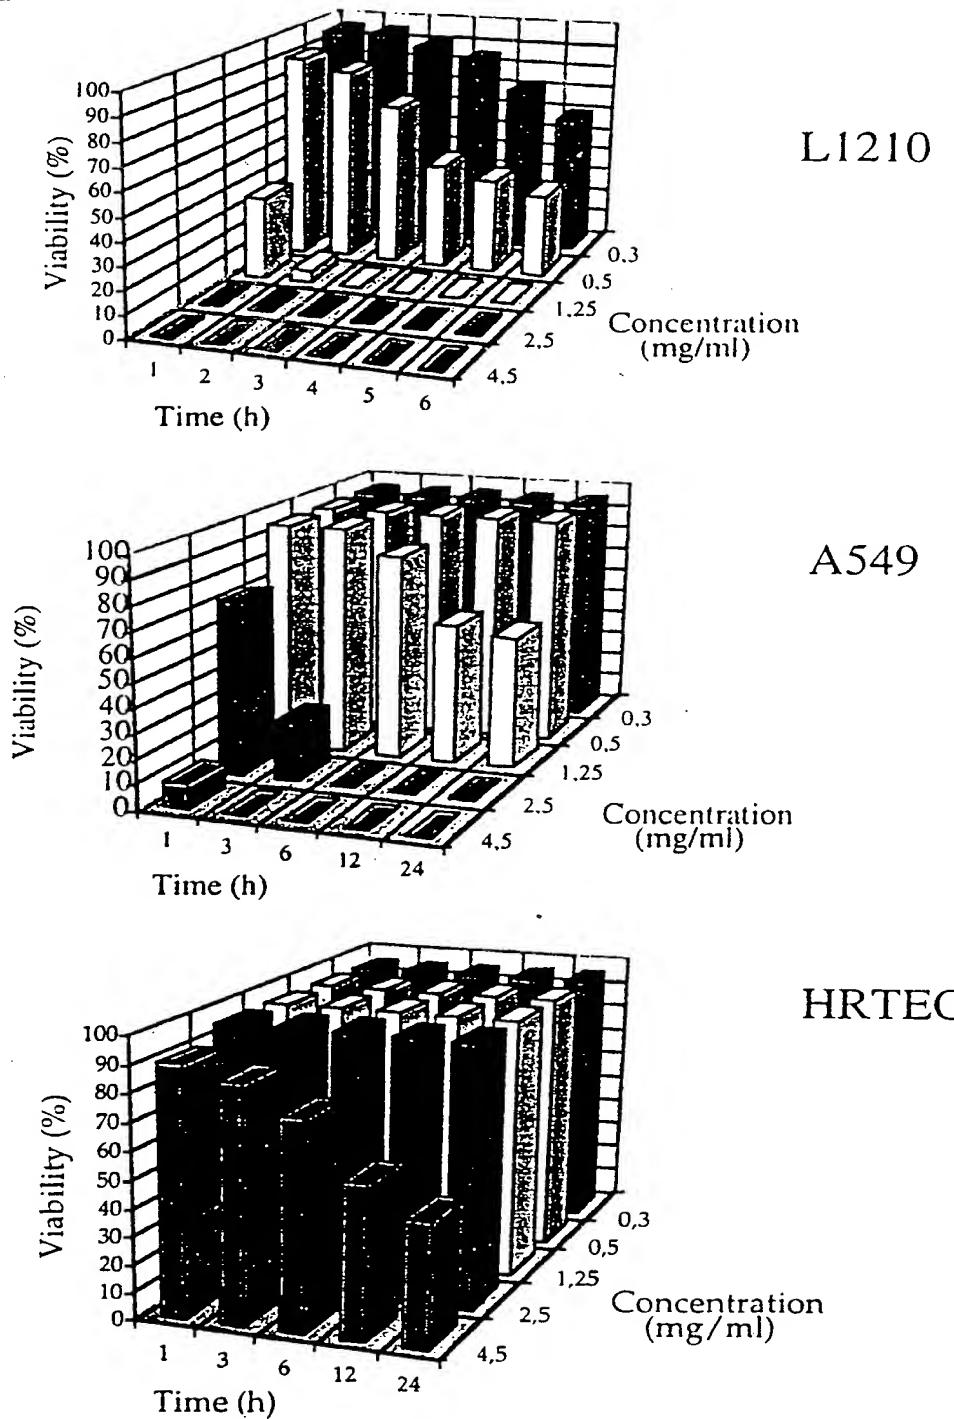


Fig. 1B (I)

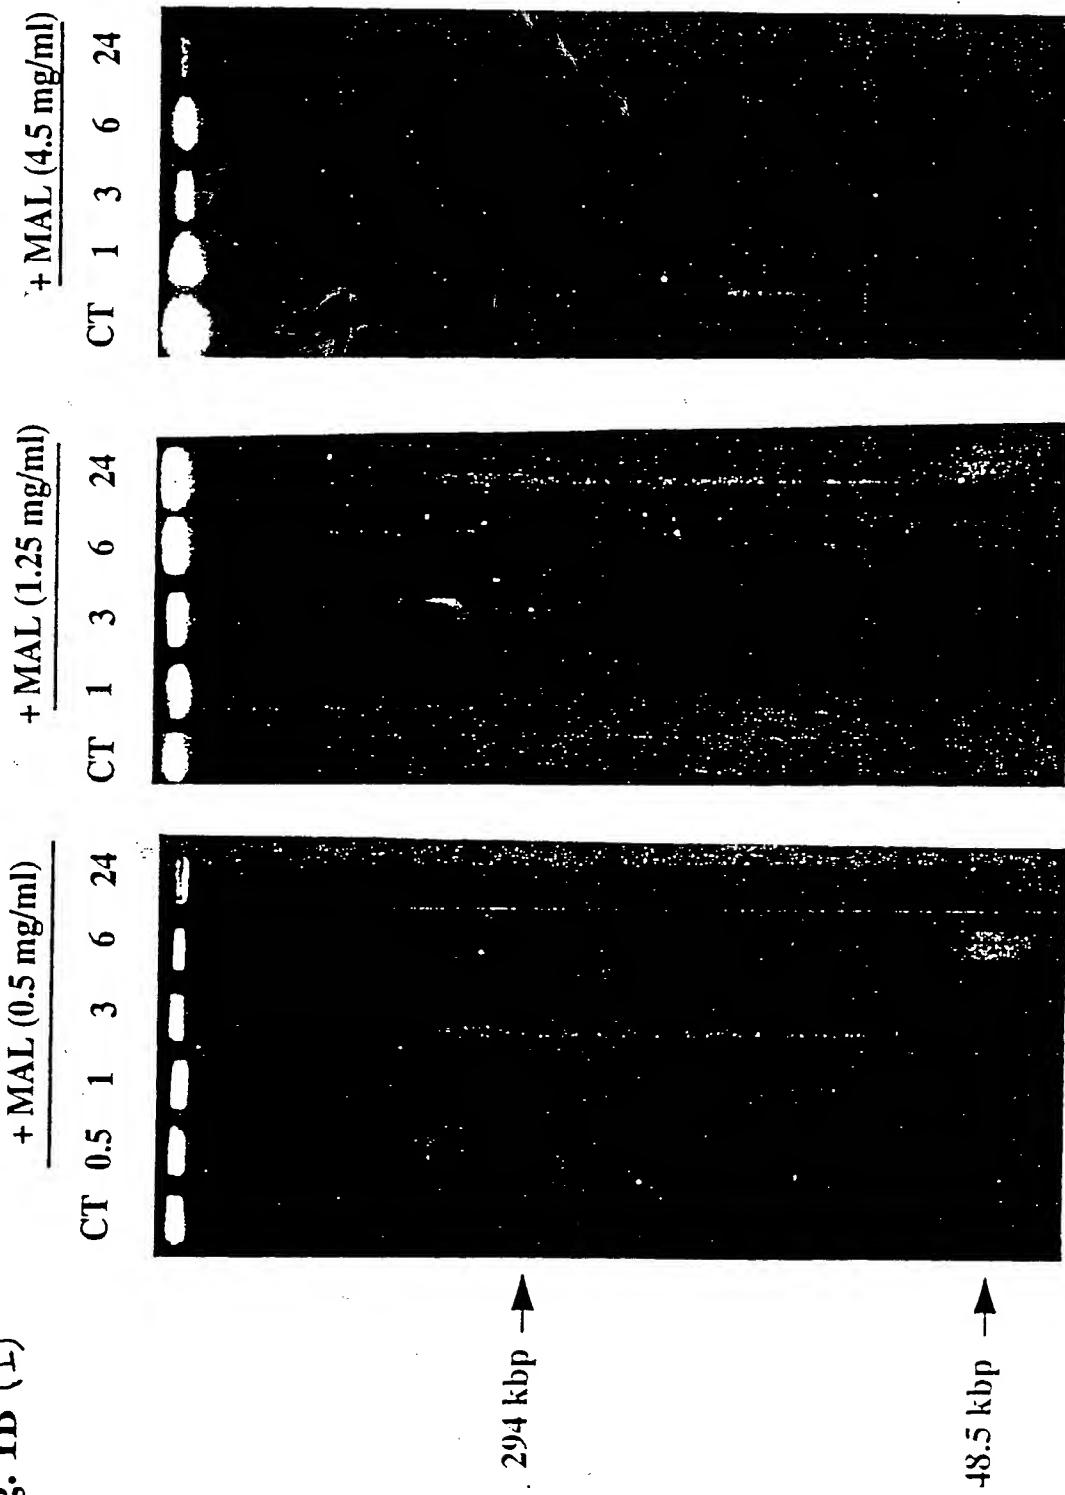

L1210

A549

HRTEC

09/555270


PCT/IB98/01920

WO 99/27967

Fig. 1B (II)

+ MAL (0.5 mg/ml)

CT 0.5 1 3 6 24 CT 1 3 6 24

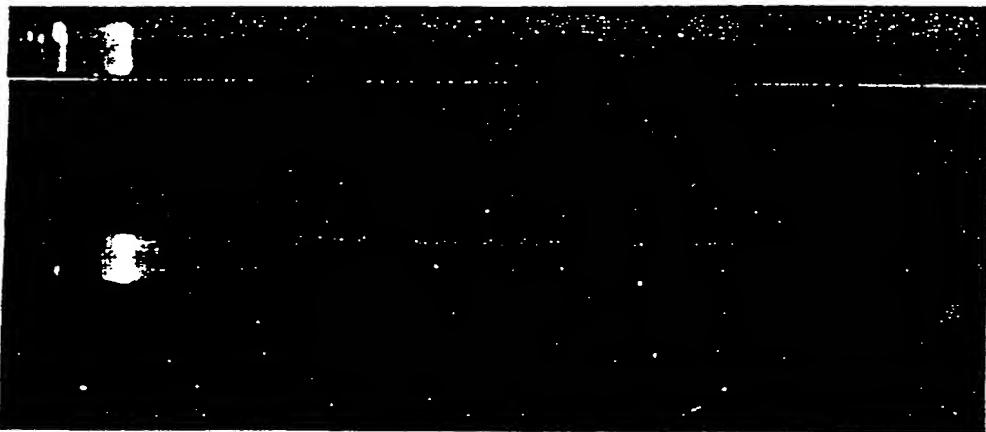

1033 →

394 →

+ MAL (1.25 mg/ml)

CT 0.5 1 3 6 24 CT 1 3 6 24







L1210

A549

HRTEC

Fig.2A

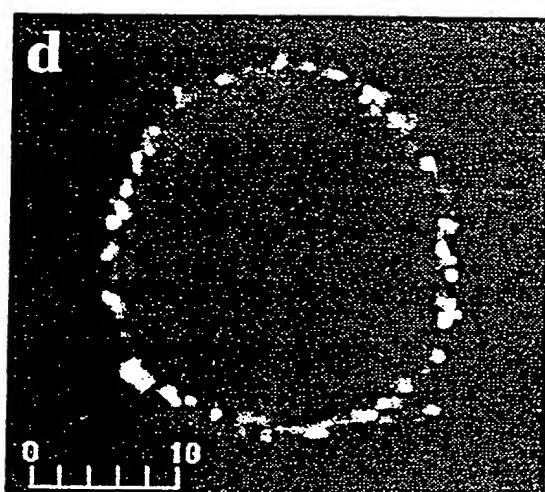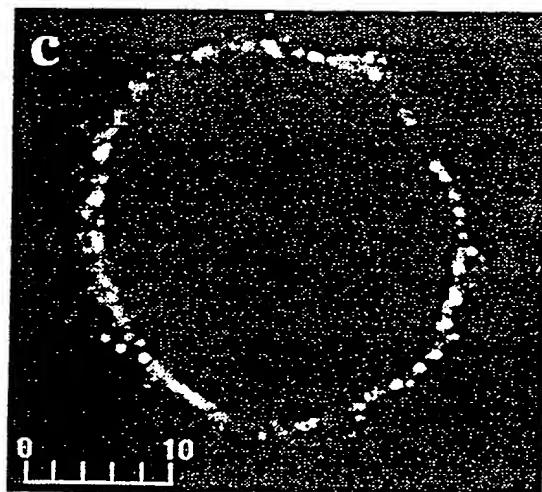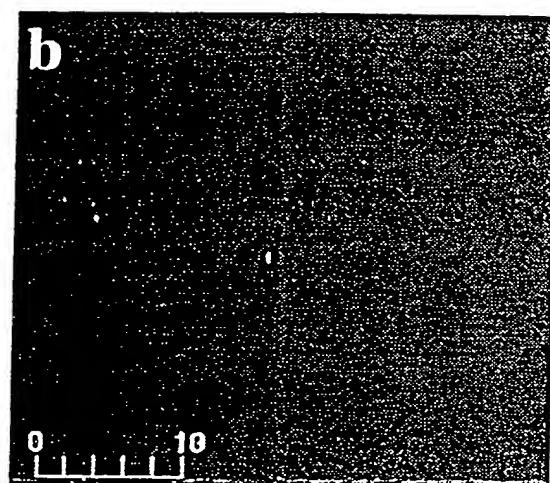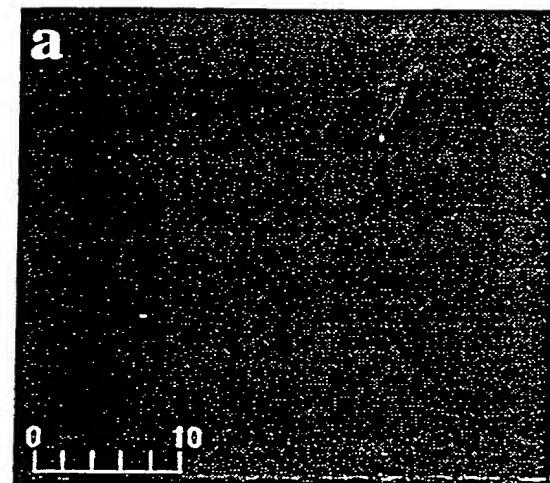

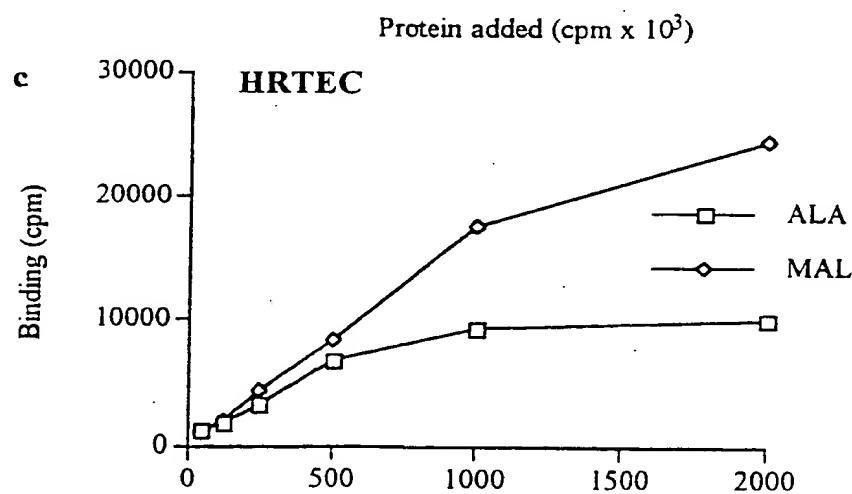
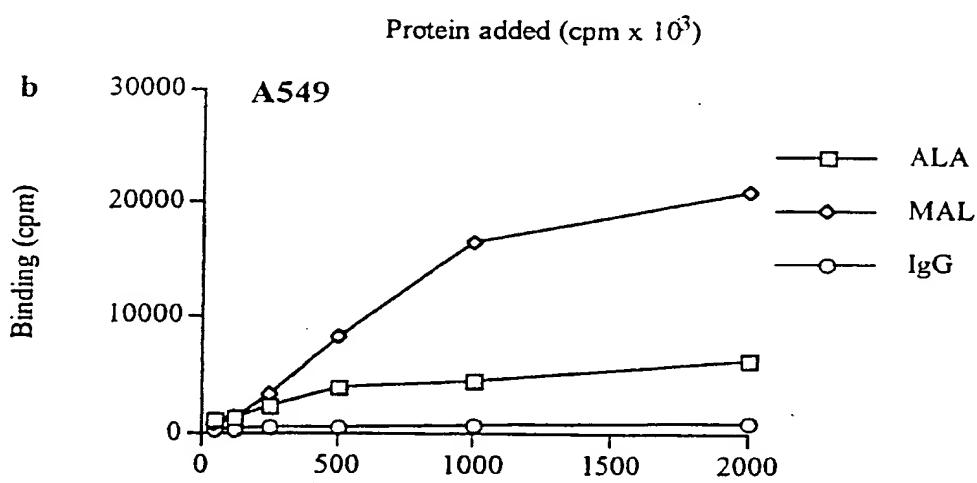
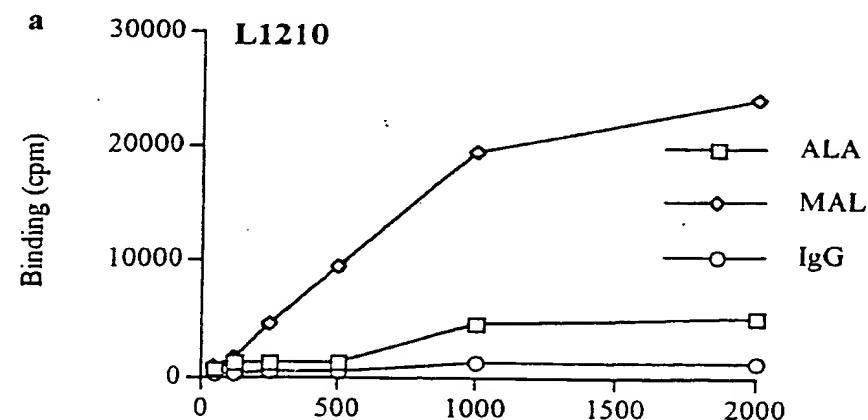


Fig.3.

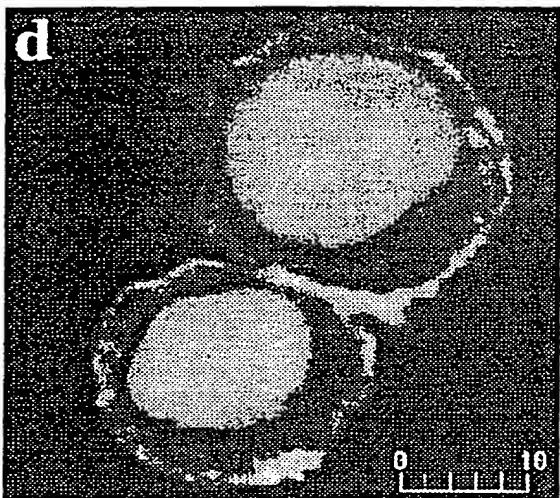
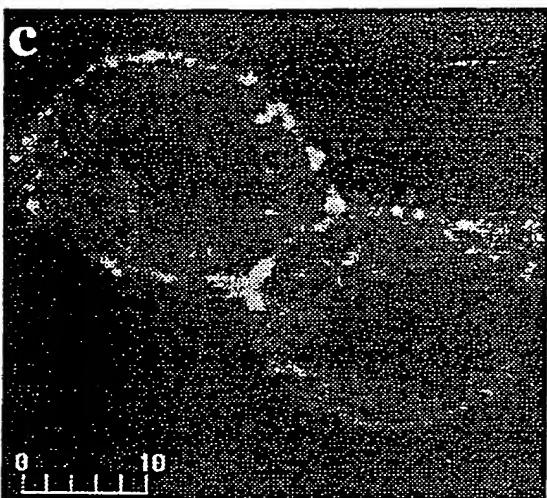
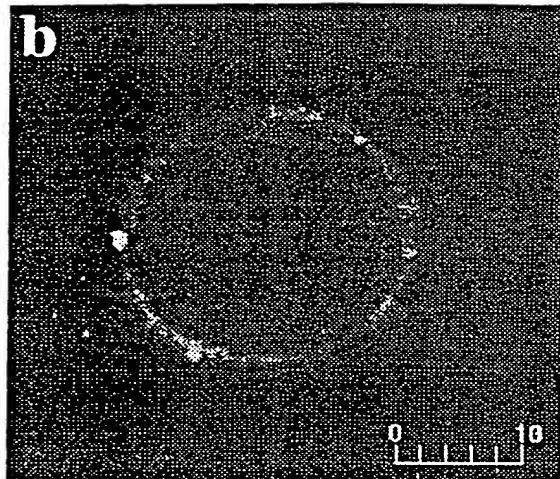
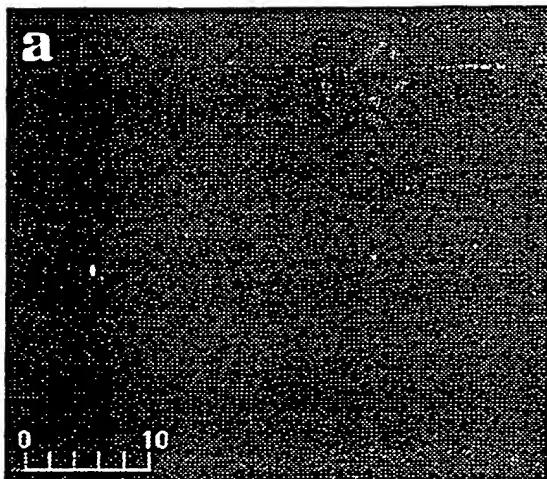


Fig. 4


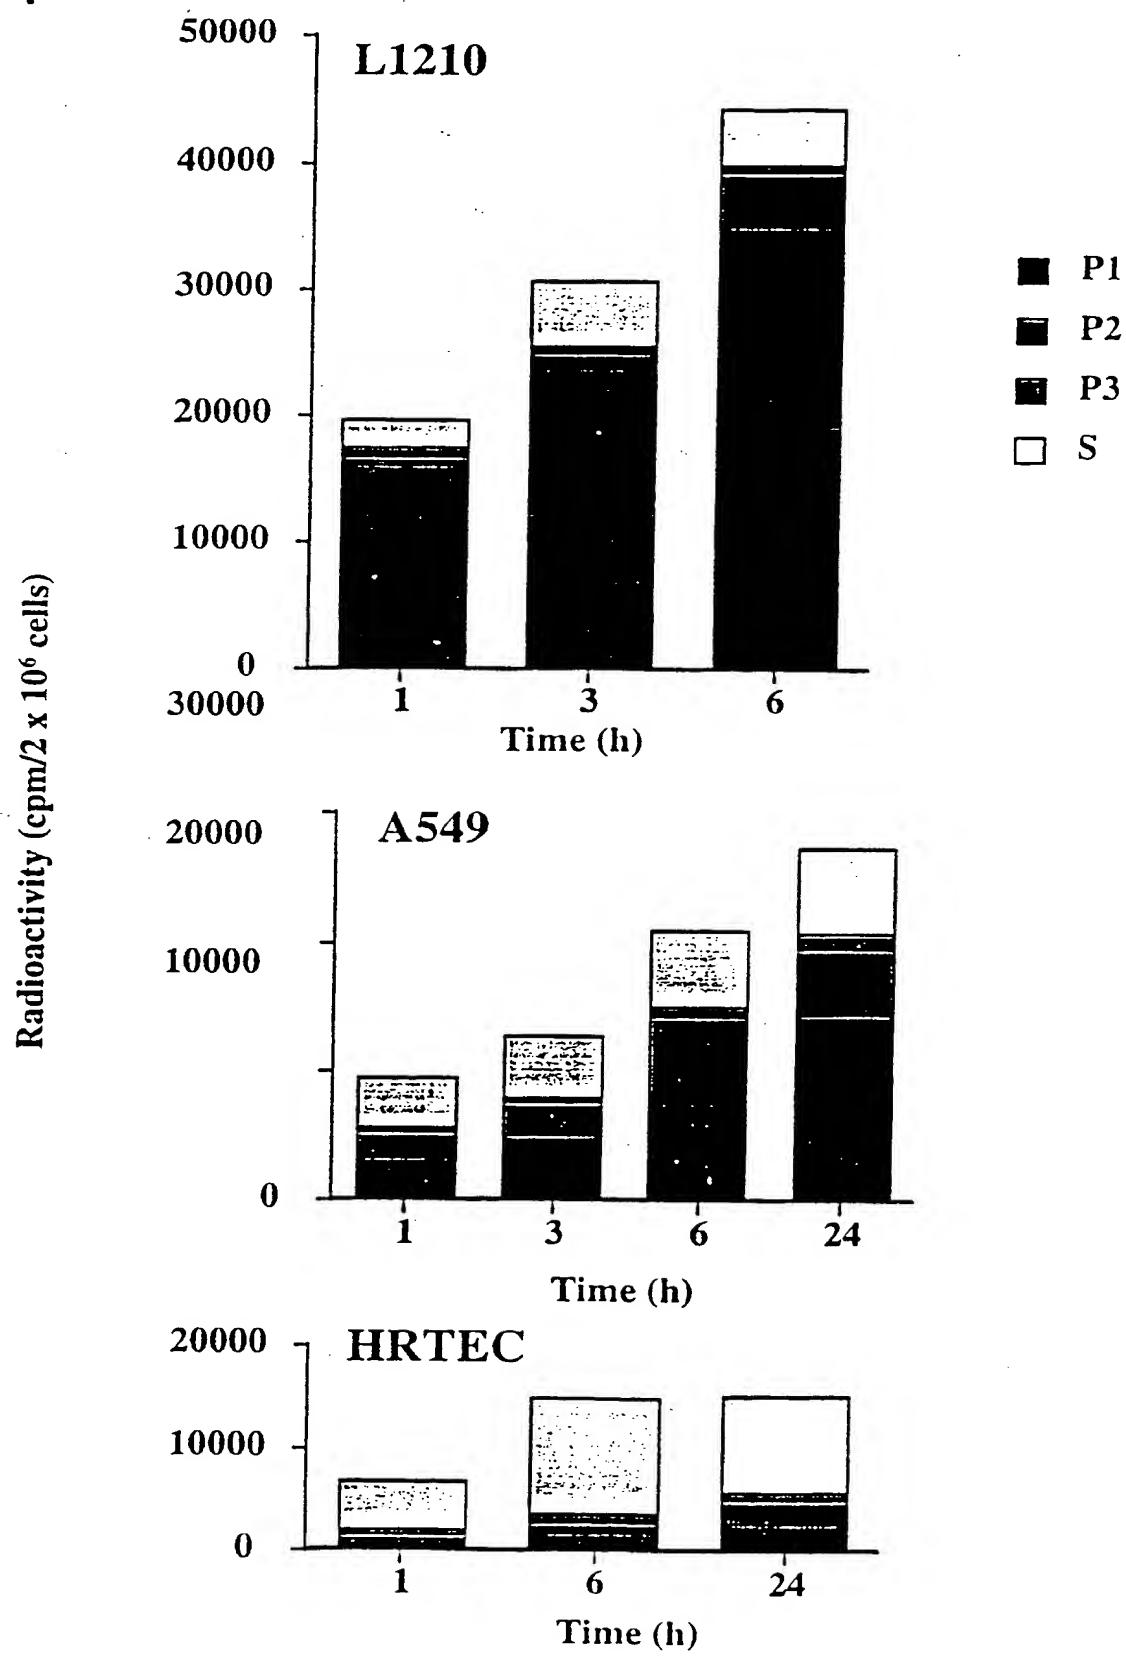


Fig. 5

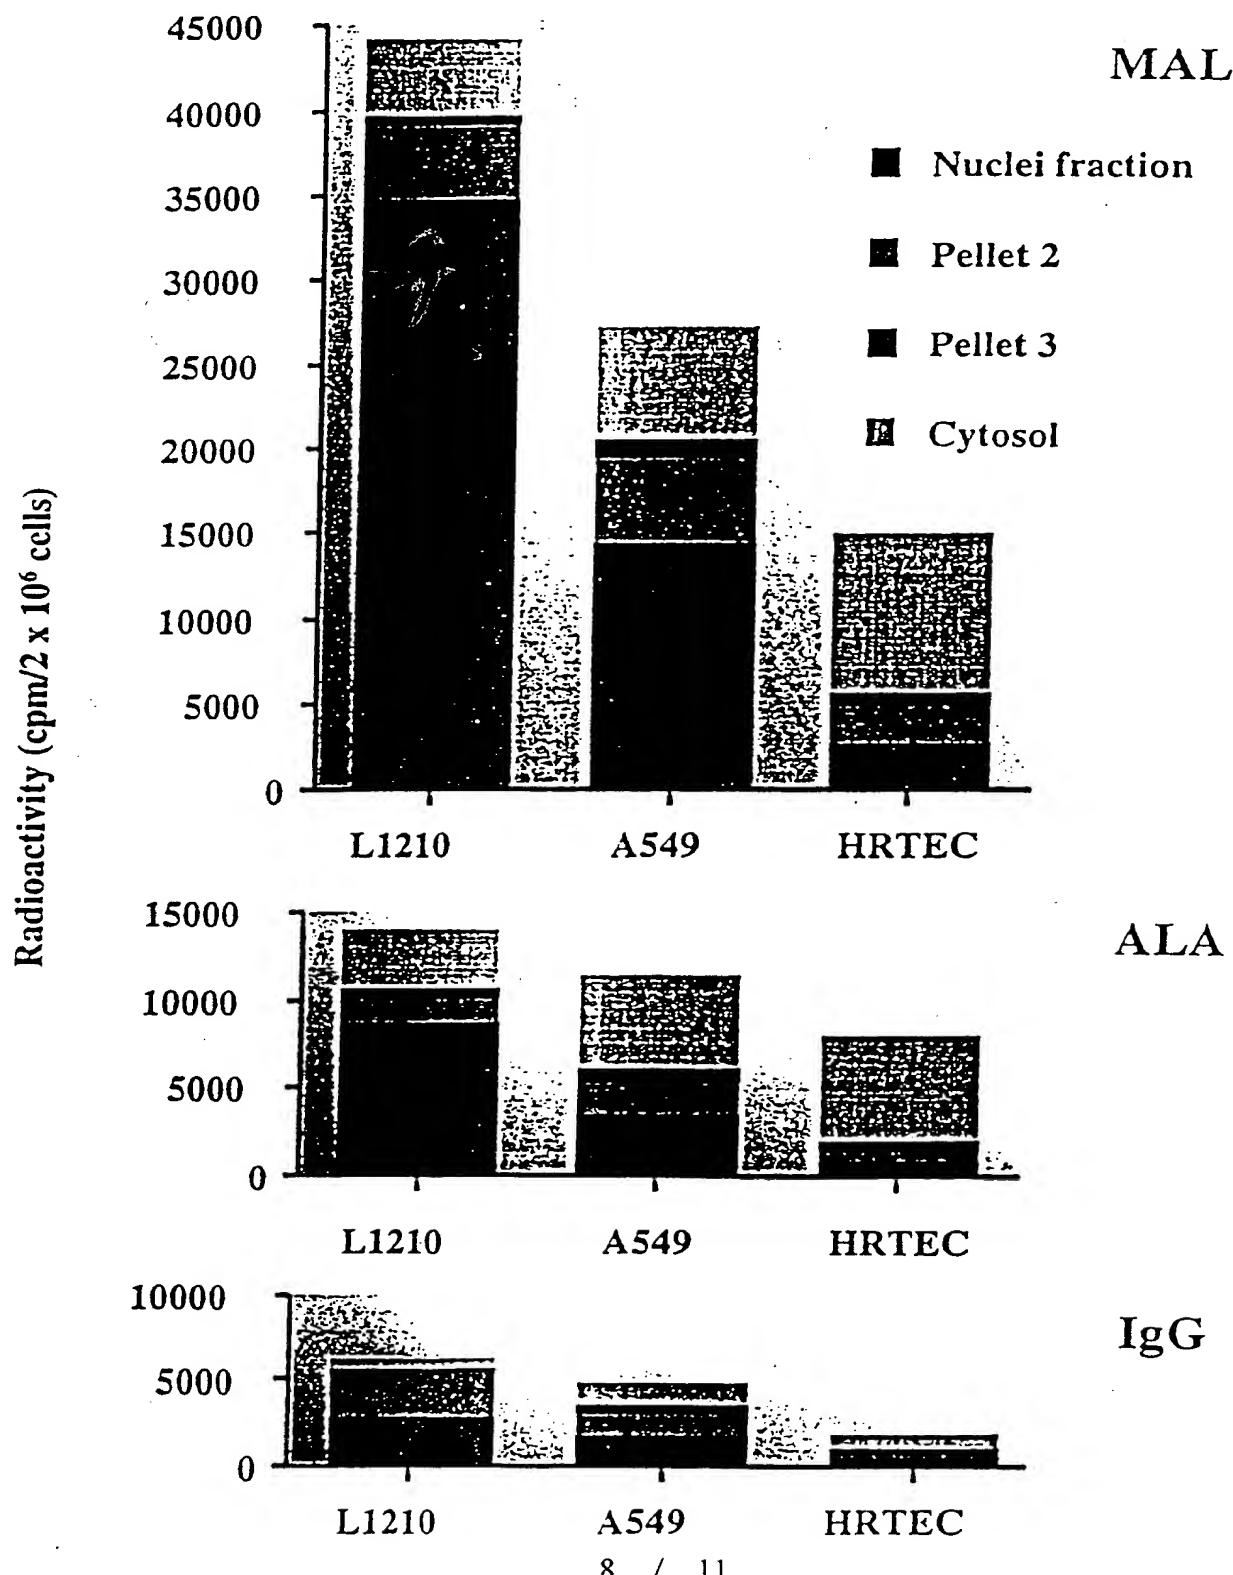


09/555270

PCT/IB98/01920

CT
MAL
+WGA



CT
MAL
+WGA

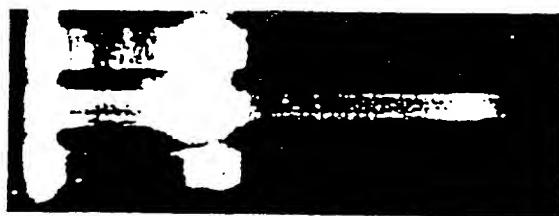

CT
MAL
+WGA



Fig. 6

CT
MAL
+WGA



HRTEC

A549

L1210

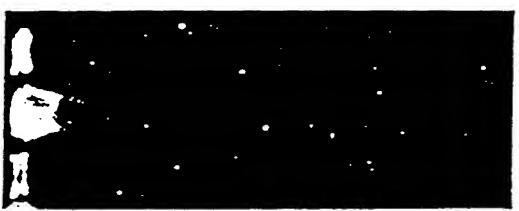


Fig. 7


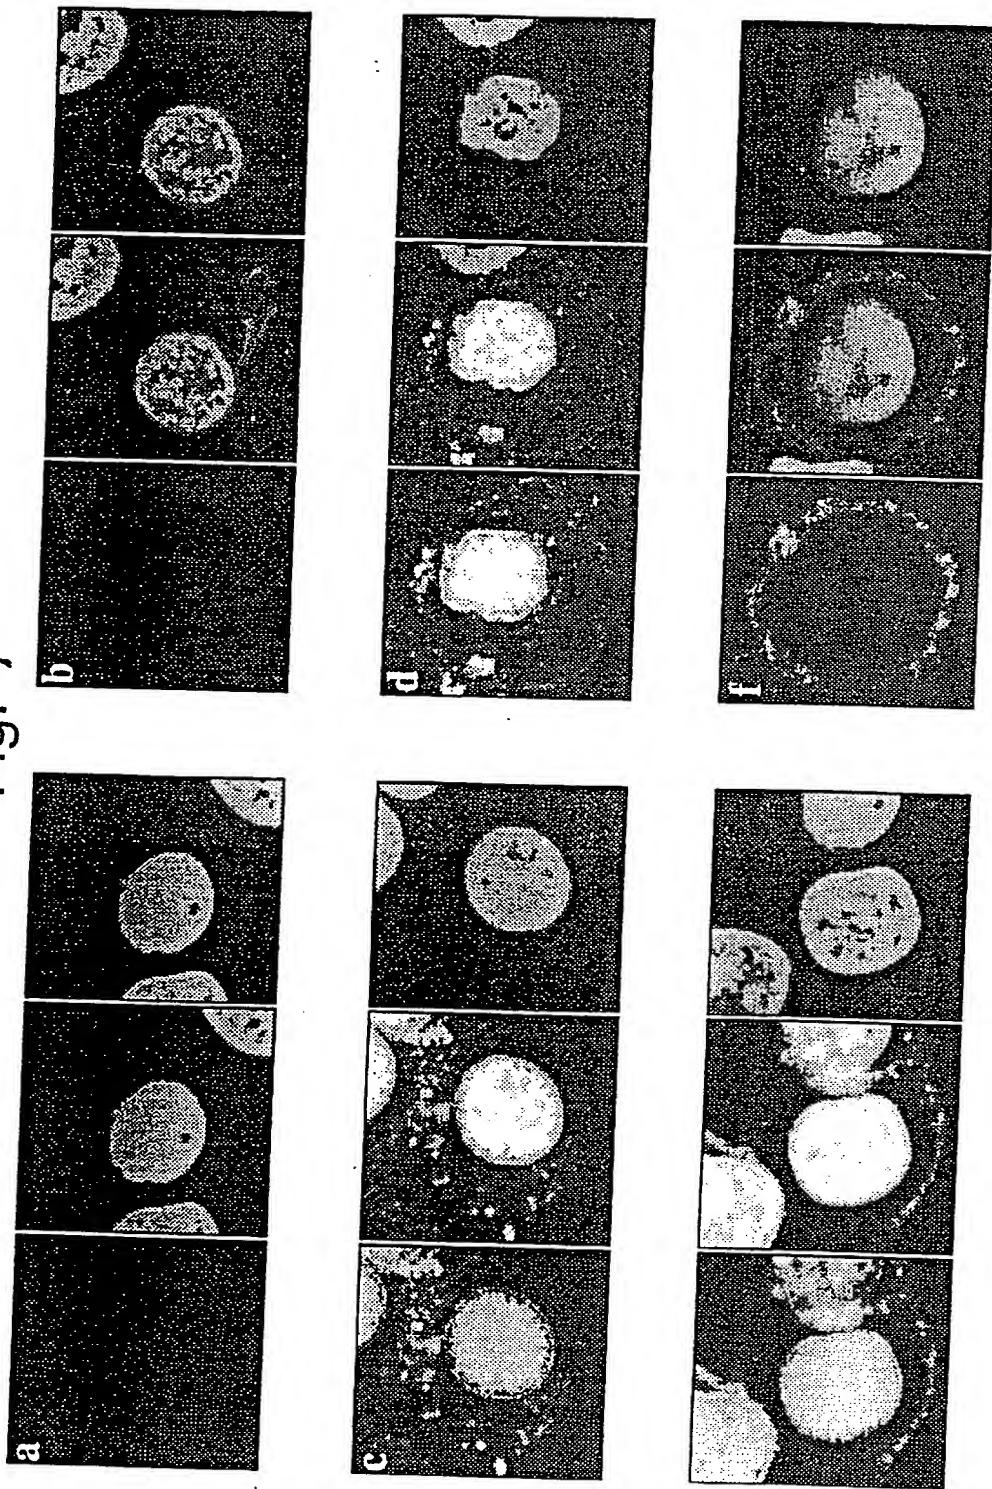


Figure 8

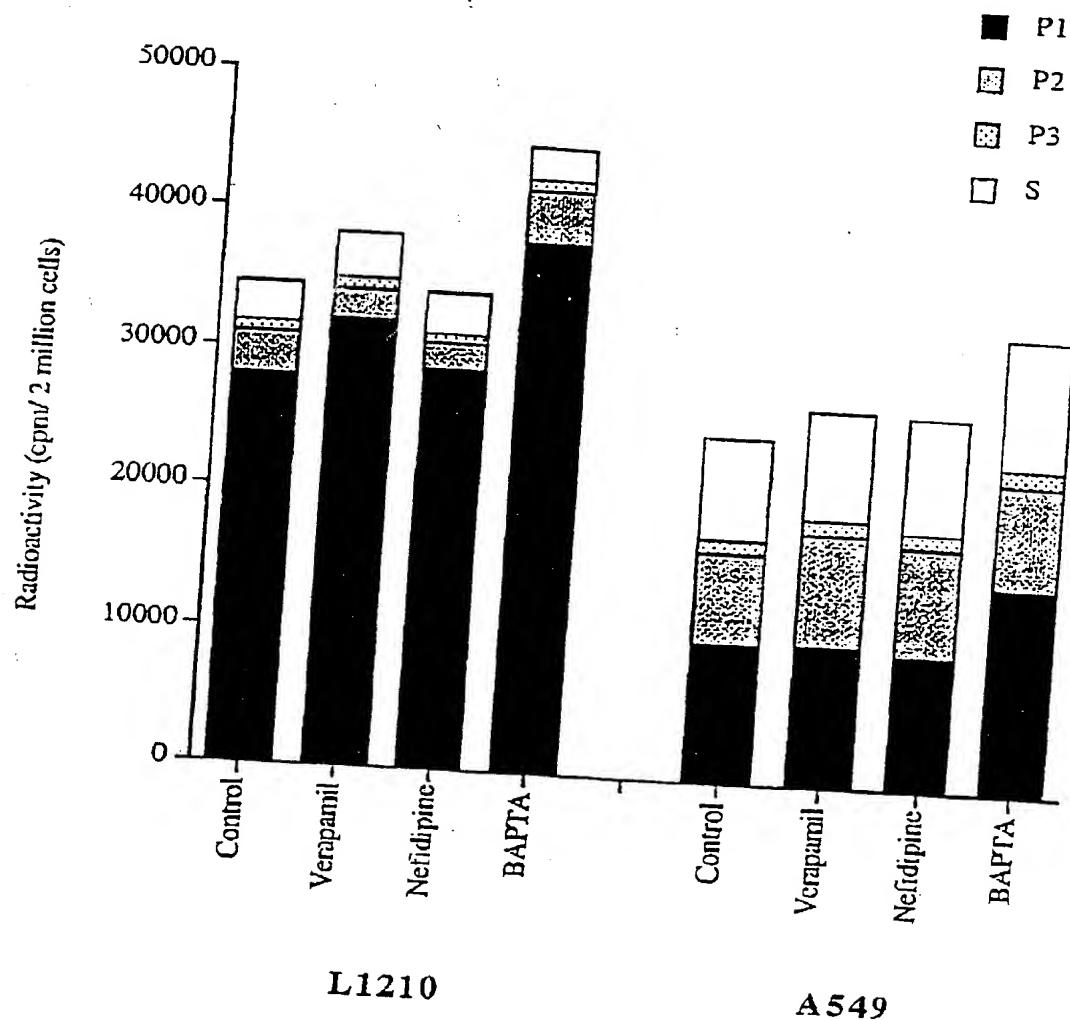

L1210

A549